

De-embedding with the WavePulser 40iX

TECHNICAL BRIEF

*Peter J. Pupalaikis and
Kaviyesh Doshi*

October 27, 2025

Summary

The WavePulser40iX offers many de-embedding methods. This technical brief explores these methods and helps the reader understand what he or she needs to provide to the instrument to obtain the best results.

Introduction

In signal integrity analysis, when measuring the S-parameters of a device under test (DUT), it is a rare circumstance when the DUT has the same connectors as the measurement instrument. The connector type for the WavePulser40iX high-speed interconnect analyzer is a 2.92mm female coaxial connection at the end of the user-supplied cables, and while these connectors are quite popular in the microwave community, most devices that are tested for signal integrity would not have this connector type. For this reason, generally extra circuitry exists in between the WavePulser and the DUT which, at a minimum, provides the change from the standard microwave connectors to other types. If this extra circuitry were completely transparent, meaning it does not affect the measurement, then it could be ignored. Most often, this is not the case, and it is desirable to remove this extra circuitry from the measurement. This is where de-embedding comes in. Simply stated, de-embedding is the act of removing extra circuitry surrounding the DUT that is often present for the sole purpose of making the measurement.

De-embedding Types Supported

The WavePulser40iX supports many different de-embedding methods. These methods fall into four broad categories:

- Calibration methods
- Time-domain methods
- Traditional frequency-domain methods
- 2X Thru, 1X Reflect (Short/Open) and 2X Thru with Gating (Impedance Corrected)

Calibration methods are methods by which various known standards are attached to a fixture and raw measurements are made. These measurements are called raw because they are measurements of the standards through the fixture. By comparing the measurements made in this way to the definitions of the standards, error terms can be generated which are used to calculate DUT measurements, thus de-embedding the fixture. Another calibration method is to take raw measurements of known standards through a section of trace to define the standard at the end of the trace. Usually, the trace is on the fixture itself, and each trace to the standard is carefully constructed to be as identical as possible to each other and to the actual connection to the DUT. Performing a calibration with the standard defined in this manner enables the de-embedding of the trace during the measurement of the DUT.

All the calibration methods can be applied directly or as a second-tier calibration. This is the subject of another technical brief. [1]

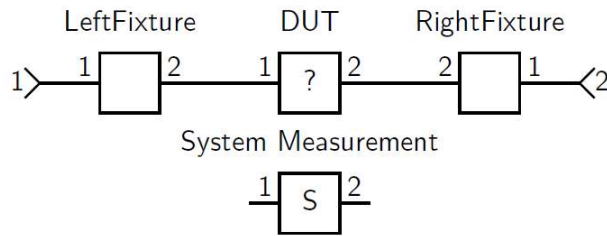


Figure 1: Simple adapter de-embedding

Time-domain methods include time-gating, also called port extension, and *peeling* methods using the information provided by the impedance trace. Armed with some knowledge or assumptions about the loss of a small section of transmission line between the instrument ports and the DUT, an approximation of the line using small sections with the measured impedance allows for the development of a model of a de-embedding structure that can be de-embedded using the frequency-domain methods. This is also the subject of another technical brief. [2]

Frequency-domain methods are most commonly used for de-embedding. All the frequency domain methods solve a problem stated in a basic way:

Given a system known to consist of fixture elements, whose S-parameters are known and a DUT whose S-parameters are unknown, solve for the S-parameters of the DUT given a measurement made of the entire system.

An example of a de-embedding problem posed in this manner is shown in Figure 1. Here, a measurement has been made of a system consisting of a left fixture, a DUT and a right fixture. The fixture S-parameters are known, as are the S-parameters measured of the entire system. In fact, this is an example of how all de-embedding problems are posed within the open-source Signal Integrity software in [3]. While the open-source software treats all de-embedding problems in the same manner, mathematically, this is actually a special case called adapter de-embedding (see [4]). Most are used to solving this type of problem using transmission parameters, or T-parameters. The steps would be, for each frequency:

1. The S-parameters of the fixtures and system are converted to T-parameters, the two fixtures and the system.
2. The inverse of the fixture T-parameters is multiplied from the left and the right by the system Tparameters (keeping in mind the port orientation of the fixtures).
3. The result is converted back to S-parameters.

For most engineers, this is the easiest way to conceptualize the solution. However, the adapter de-embedding method is the method used for this type of problem when you are fortunate enough to have the problem posed as two-port devices between the instrument ports and the DUT ports.

If a traditional frequency-domain de-embedding problem cannot be posed in the manner required for adapter de-embedding, then fixture de-embedding must be utilized. This method, which assumes one large fixture between all ports of the measurement instrument and all ports of the DUT, is capable of solving any traditional de-embedding problem, but some extra work might be required to generate the fixture. This will be discussed later in this document.

Adapter and Fixture De-embedding Selection

The basic setup menu is shown in Figure 2. This menu provides the bare minimum information required to perform a measurement. Advanced setup is accessed by clicking on any of the small plus signs scattered throughout the setup, which indicates advanced setup possibilities when expanded. Although the advanced setup controls are hidden, nearby text on the menu indicates the configuration status.

For example, the status of the hidden fixture and adapter de-embedding settings is shown to be "disabled" by the text inside the green box in Figure 2.

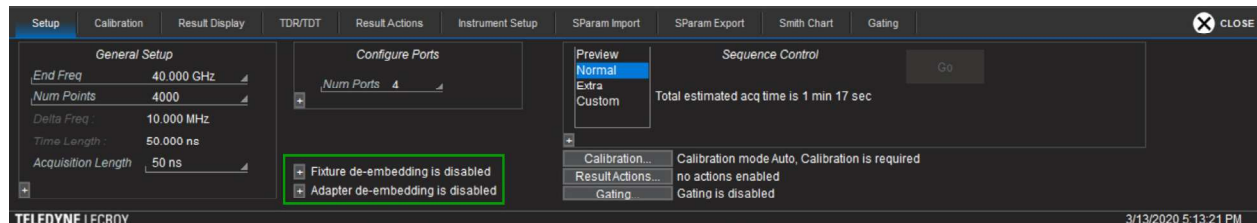


Figure 2: WavePulser40iX basic setup menu

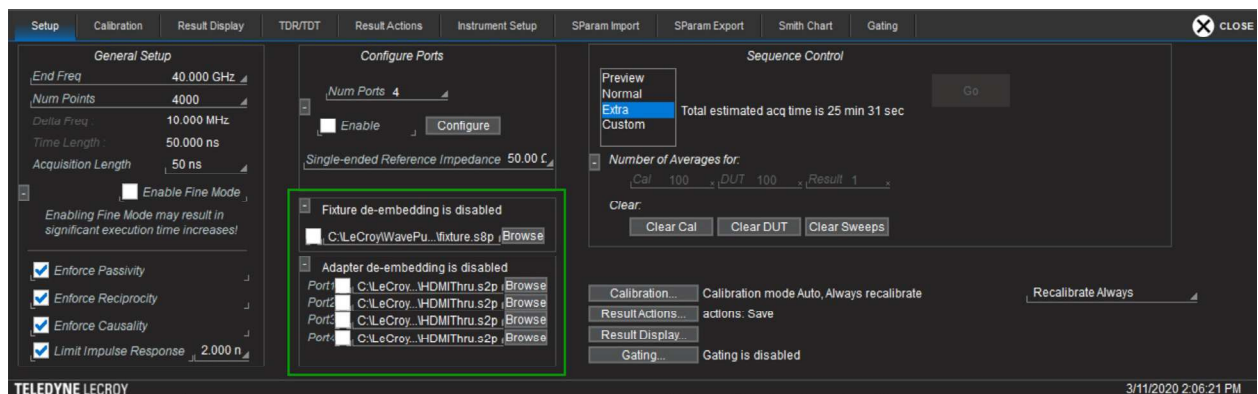


Figure 3: WavePulser40iX advanced setup menu

If any plus sign is clicked, the setup menu expands, as shown in Figure 3. Here, one can see that, among other advanced settings, the fixture and adapter de-embedding sections are expanded. The adapter de-embedding area shows a list for each physical port of the WavePulser. For each port, a checkbox is provided that enables the de-embedding of an adapter on the specified port and shows the name of the two-port s-parameter file containing the S-parameters to de-embed. For adapter de-embedding, the assumption is always a two-port, single-ended device with port 1 of the adapter connected to the physical WavePulser port and port 2 connected to the DUT.

Fixture de-embedding operates in a similar manner, but in this case, the assumption is a fixture with twice the number of single-ended ports as the DUT where, for P DUT ports, ports 1 to P are connected to the physical WavePulser ports and ports $P + 1$ to $2 \cdot P$ are connected to ports 1 to P of the DUT.

This is shown schematically in Figure 4, which shows it is possible to utilize both adapter and fixture de-embedding at the same time, provided one keep in mind the de-embedding schematic that is assumed.

Fixture De-embedding Details

When the de-embedding cannot be accomplished through adapter de-embedding, fixture de-embedding can be utilized to solve any de-embedding problem. This is not obvious to some because, for example, Figure 4 is not shown in the manner that most people visualize their de-embedding problem. It can be

seen though that as the fixture connects all WavePulser ports to all DUT ports, any arbitrary circuit can be placed inside the fixture to solve any problem posed. That being said, sometimes the devices to be de-embedded need to be manipulated into the form of a fixture for use. This manipulation can be performed with the free open-source software called *Signal Integrity* offered by Teledyne LeCroy (see [3] for the download location).

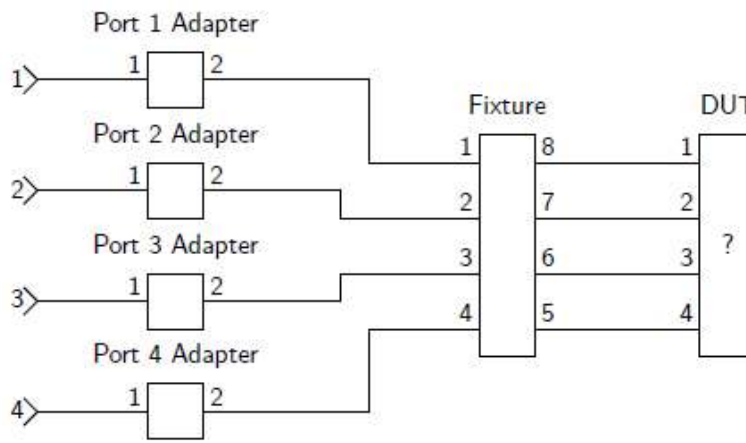


Figure 4: Fixture and adapter de-embedding circuit

To illustrate the creation of a fixture suitable for use in the WavePulser, an example is provided in Figure 5. A common example is the measurement of a four-port DUT whereby two four-port fixtures are used on each end, as shown in Figure 5a. This example was created in the *Signal Integrity* software. If system S-parameters (the measured S-parameters of this four-port system) were provided, the application would be able to perform the de-embedding operation and recover the S-parameters of the DUT. In this example, however, we will concern ourselves with the creation of the fixture file required for use in the WavePulser application. Since the DUT has four ports, the fixture file has eight, as explained previously. The easiest way to design a proper fixture file is to construct exactly the schematic as in Figure 5a, then move the DUT element away and connect ports to the newly unconnected fixture locations, making sure that, for a P -port DUT, the new ports are numbered $P + 1$ for DUT port 1, $P + 2$ for DUT port 2, etc., up to $2 P$ for DUT port P . Then, delete the DUT element that moved away (but was retained to check the port numbering) and compute the S-parameters of the resulting schematic that is shown in Figure 5b. The *Signal Integrity* application allows the specification of the number of frequency points and end frequency, thus determining the frequency resolution of the fixture. This must be chosen properly for your application and should, at a minimum, contain the expected number of frequency points and end frequency that are planned to be used for the de-embedded DUT calculation.

It is easy to become disoriented with the fixture de-embedding situation, so Figure 5c is provided, which shows the fixture constructed from Figure 5b, but in the same orientation as the fixture shown in Figure 4. The fixture calculated can be solved with the *Signal Integrity* software using the schematic shown in Figure 5d, given four port s-parameter measurements of the entire system. Of course, here the goal is to create the fixture file for the WavePulser, as shown in Figure 3 where the file Fixture.s8p is provided for fixture de-embedding.

De-embedding Math

The complete description of the mathematics used for de-embedding is provided in [4, 5]. Here, the equations for de-embedding a $2 \cdot P$ -port fixture with S-parameters F from a P -port unknown DUT with S-parameters S are provided without justification. Given known system S-parameters S_m for a fixture de-embedding arrangement Left_Fixture.s4p, DUT Right_Fixture.s4p, Left_Fixture.s4p, Right_Fixture.s4p:

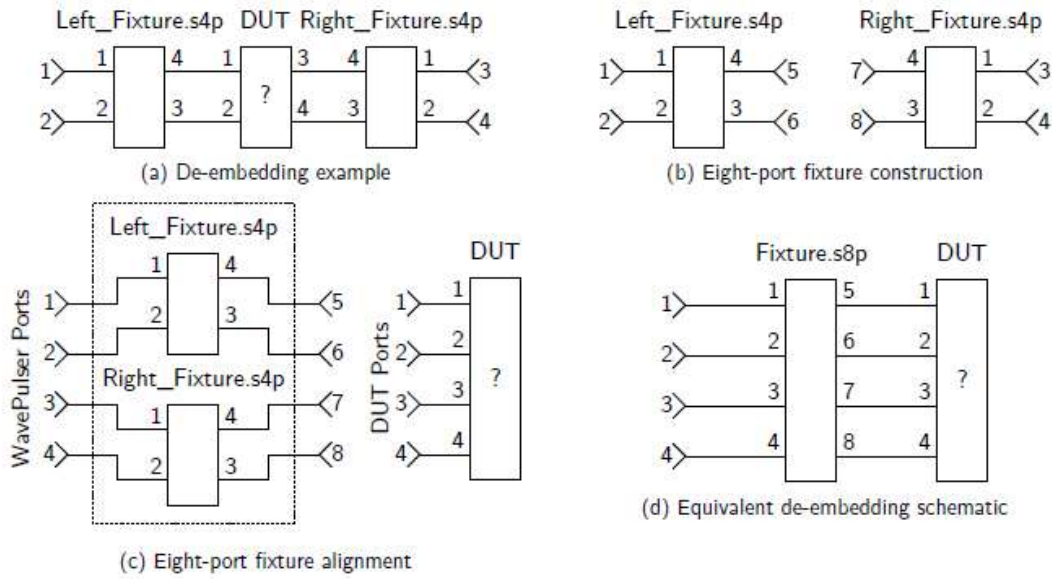


Figure 5: Fixture de-embedding examples

as shown in Figure 5d, the fixture S-parameters are partitioned in the block matrices:

$$\mathbf{F}_{2 \cdot P \times 2 \cdot P} = \begin{pmatrix} \mathbf{F}_{11} & \mathbf{F}_{12} \\ \mathbf{F}_{21} & \mathbf{F}_{22} \end{pmatrix}$$

$P \times P$ $P \times P$
 $P \times P$ $P \times P$

Solving for the unknown DUT S-parameters using the solution established in [4] results in:

$$\mathbf{B} = \mathbf{F}_{12}^{-1} \cdot (\mathbf{S}_m - \mathbf{F}_{11}),$$

$$\mathbf{A} = \mathbf{F}_{21} + \mathbf{F}_{22} \cdot \mathbf{B},$$

$$\mathbf{S} = \mathbf{B} \cdot \mathbf{A}^{-1}.$$

This fixture de-embedding equation is very adaptable, and in fact, becomes the adapter de-embedding solution when the block matrices \mathbf{F}_{11} , \mathbf{F}_{12} , \mathbf{F}_{21} , and \mathbf{F}_{22} are constructed as diagonal matrices with the adapter sparameters placed on the diagonal in port order. In other words, with adapter S-parameters of \mathbf{A}_p for each port (with $\mathbf{A}_p = \begin{pmatrix} 0 & 1 \\ 1 & 0 \end{pmatrix}$) used as the S-parameters when an adapter is not present), the block matrices are formed as:

$$\mathbf{F}_{rcpp} = \mathbf{A}_{p_{rc}},$$

where both $r \in 1, 2$ and $c \in 1, 2$.

2X Thru, 1X Reflect (Short/Open) and 2X Thru with Gating (Impedance Corrected)

The **2X Thru** de-embedding method is a powerful and widely adopted technique for high-speed PCB interconnect characterization. It uses a symmetrical test structure—two fixtures directly connected to each other, as shown in Figure 6—to isolate and remove fixture effects from measurements. By eliminating the DUT and focusing on the fixture itself, engineers can extract precise S-parameters and achieve highly accurate signal integrity analysis.



Figure 6: 2X Thru test structure

Figure 7 shows the WavePulser user interface for traditional, 4-port 2X Thru de-embedding. The **2X Thru** de-embedding feature uses the S-parameter measurement of a 2X Thru structure to compute the S-parameters of each half of the fixture. These "split" S-parameters are then applied to the de-embedding interface to isolate and remove fixture effects, enabling accurate characterization of the DUT. The 2X Thru method excels at high frequencies, where even minor discontinuities can disrupt signal integrity. Fully compliant with IEEE P370, it delivers precise, repeatable results—making it an essential tool for modeling and validating high-speed interconnects in advanced electronic designs.

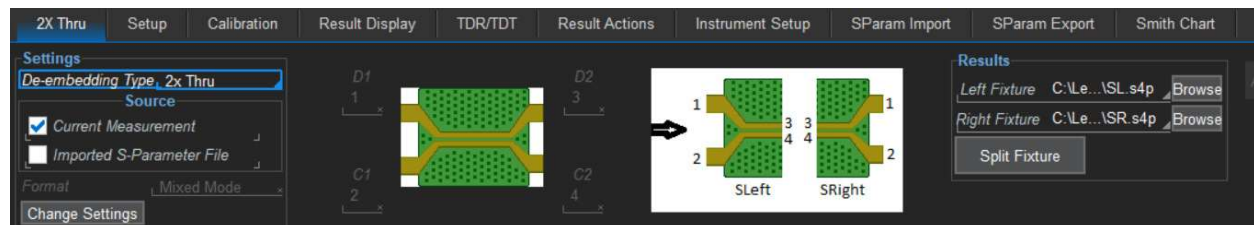


Figure 7: WavePulser 40iX 2X Thru setup using current measurement

In scenarios where the back-to-back fixture design described above is not possible, an alternative approach is to leave one end of the fixture open and measure it as a 1X Open, as shown in Figure 8. The **1X Short/Open** de-embedding method utilizes the measurement of an open structure to determine key gating parameters such as length and loss. These parameters are then used to de-embed the fixture via the WavePulser Gating feature.

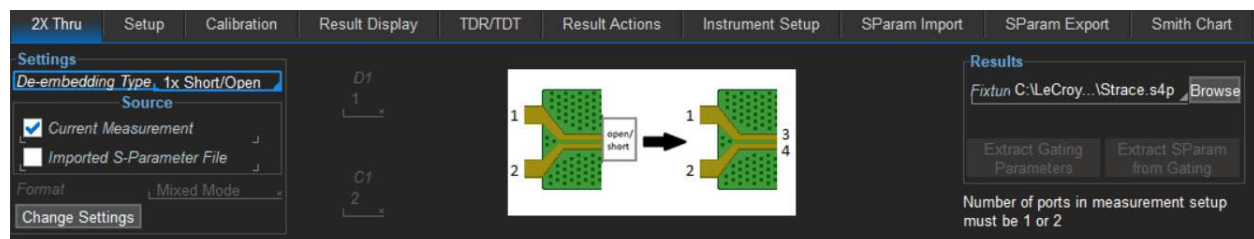


Figure 8: WavePulser 40iX with 1X Short/Open setup using current measurement

The **2X Thru with Gating** (impedance corrected) method represents an advanced enhancement of the basic 2X Thru de-embedding technique. This approach incorporates impedance profile measurements

used to calculate gating parameters that refine the accuracy of fixture removal. Leveraging the Time Domain Reflectometry (TDR) technology of the WavePulser, this method enables highly precise impedance characterization. As a result, the de-embedding algorithms deliver significantly improved performance and reliability, particularly in complex signal environments. Unlike basic 2X Thru de-embedding, which assumes ideal fixture behavior, the impedance-corrected version accounts for real-world variations in characteristic impedance, reflections, and discontinuities in the measurement setup.

See the application note, *Mastering WavePulser 40iX 2X Thru De-embedding*, for traditional 2X Thru de-embedding measurement and verification procedures.

Conclusion

The WavePulser 40iX contains a multitude of de-embedding methods not typically found in other instruments including calibration, time-domain, frequency-domain and 2X Thru methods. Often, the problem is a simple, two-port adapter de-embedding problem. When it is not, fixture de-embedding can be used to solve any frequency domain de-embedding problem, albeit with the construction of fixture S-parameters, which are easily performed using the open-source *Signal Integrity* software.

References

- [1] P. J. Pupalais, "WavePulser40iX Second-Tier Calibration," Teledyne LeCroy Technical Brief, Mar. 2020.
- [2] P. J. Pupalais, "Time-Domain Techniques for De-embedding and Impedance Peeling," Teledyne LeCroy Technical Brief, Mar. 2020.
- [3] The *SignalIntegrity* project, <https://pypi.org/project/SignalIntegrity/> and <https://github.com/TeledyneLeCroy/SignalIntegrity/>.
- [4] P. J. Pupalais, *S-Parameters for Signal Integrity*. Cambridge: Cambridge University Press, 2020, pp. 287–290.
- [5] P. J. Pupalais and K. Doshi, "Method for de-embedding device measurements," U.S. Patent 8566058, Oct. 22, 2013.

Copyright 2025 Teledyne LeCroy, Inc. All rights reserved.